


14 August 2014

TECHNICAL RELEASE
LUZCHEM EXPOSURE STANDARD: LES-LEDNW-14

General information: Luzchem Research, Inc. produces and distributes freely these standards as a service to scientists involved in research in photochemistry, photobiology and photostability. These standards are available in Luzchem's website so that references to any of our standards can be used to define conditions of exposure, and should allow other scientists to readily replicate irradiation conditions. Luzchem has measured these exposure standards using a Luzchem SPR-4001 spectroradiometer calibrated against traceable NIST standards within the 6 months preceding the determination. To the best of our knowledge spectral information is accurate within the experimental bandwidth of 2 nm.

Lamp part number	Luzchem LED-NW	Measurement temperature	23 °C
Filter	None, direct exposure	Measurement date	14-August-2014
Filter effect determined by	Not applicable	Spectral range monitored	240 to 880 nm
Photoreactor model	EXPO-LED	Harmonic peak interference	None observed
Number of lamps and location	5 overhead lamps, approx 10 cm from target	Lamp type:	T5 Broadband
Colour Temperature	4000-4500 K	Resolved peaks	448,572 nm

LED lamps start at a shorter wavelength than their stabilized temperature and take about 5 min to equilibrate.

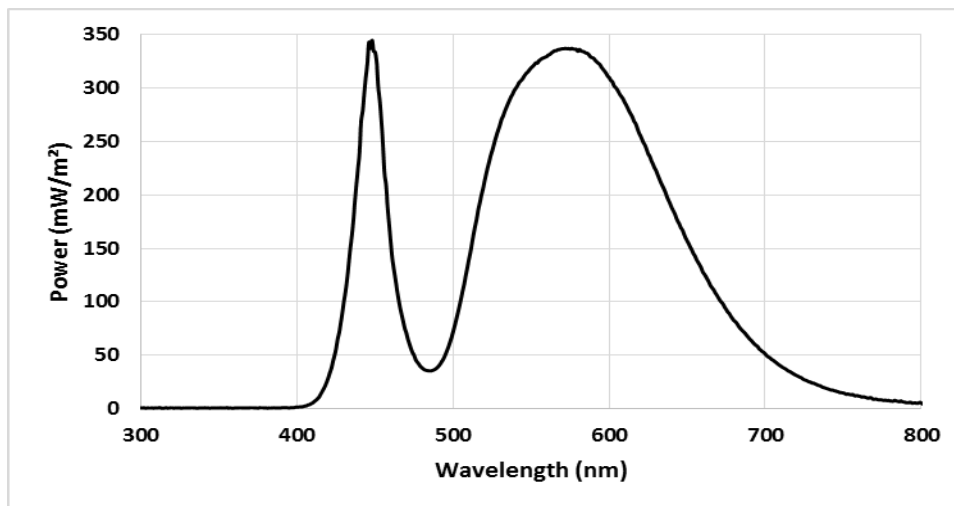

Region	Range nm ^a	Dose mW/m ²	% Energy ^b
UVA	316-400	59	<1%
Wavelength Range – Peak 1	400-485	9722	17%
Wavelength Range- Peak 2	485-700 (Broad)	45011	79%
Visible	400-700	54774	>95%
NIR	701-850	2056	<4%

The table to the left shows the energy distribution at the target, expressed as total irradiance and as a percentage of the total energy. The calculations refer to the monitored range indicated.

Integration range. ^b Within experimental error.

Luzchem Research, Inc.

Toll free 1-800-397-0977
Phone: (613) 749-2442
Fax: (613) 749-2393
E-mail: sales@luzchem.com

5509 Canotek Road, Unit 12
Ottawa, Ontario
Canada K1J 9J9
www.luzchem.com